


11.016

9.897

7.571
7.567
7.548
7.528
7.510
7.506
7.260
7.039
7.038
7.020
7.001
6.980

1.616

-0.003

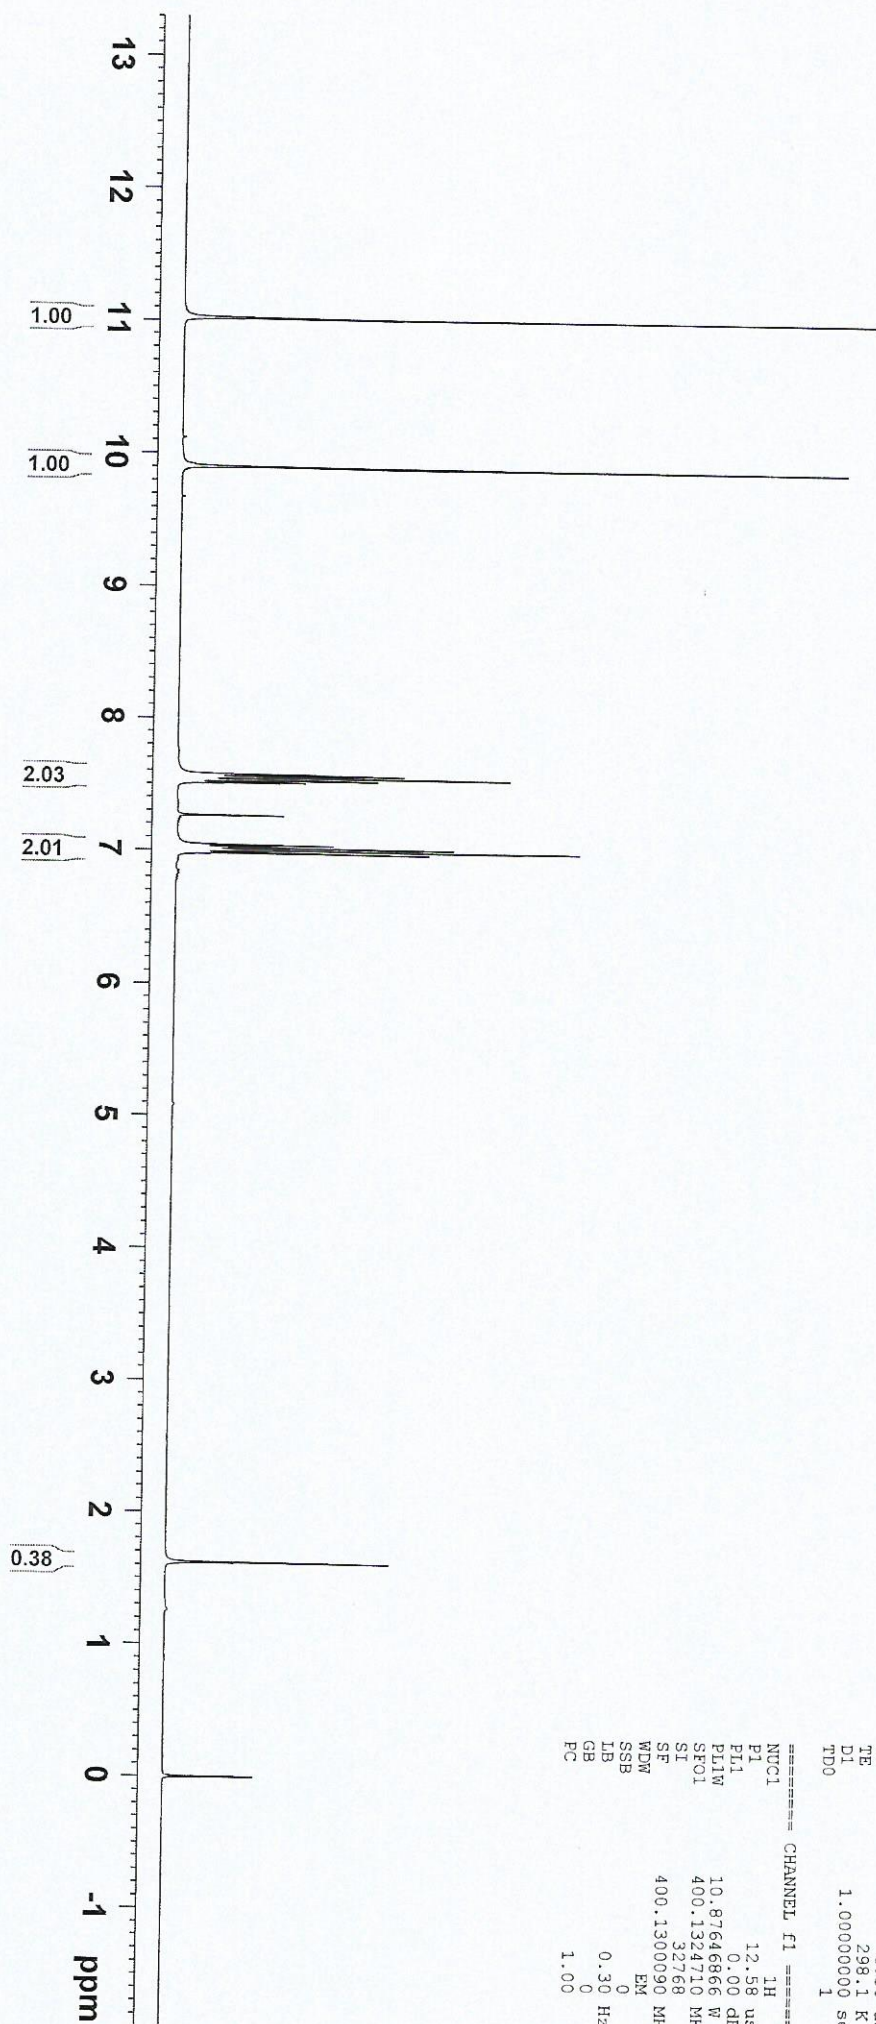

```

NAME      Sep06-2015
EXPNO     23
PROCNO    1
Date_     20150906
Time      13.42
INSTRUM   spect
PROBHD    5 mm PABBO BB-
PULPROG   zg30
TD         65536
SOLVENT   CDCl3
NS         8
DS         2
SWH        8278.146 Hz
FIDRES     0.126314 Hz
AQ         3.9584243 sec
RG         181
DE         60.400 usec
TE         298.1 K
D1         1.00000000 sec
TD0        1

===== CHANNEL f1 =====
NUC1       1H
P1         12.58 usec
PL1        0.00 dB
PL1W       10.87646866 W
SFO1       400.1324710 MHz
SI         32768
SF         400.1300090 MHz
WDW        EM
SSB        0
GB         0.30 Hz
PC         1.00
  
```