


10.524
10.523

7.839
7.835
7.820
7.816
7.546
7.542
7.528
7.525
7.524
7.521
7.507
7.502
7.260
7.020
7.002
6.982
6.961

4.058
4.042
4.026

1.903
1.887
1.868
1.852
1.105
1.092
1.086
1.074
1.063
1.055
1.045

-0.004

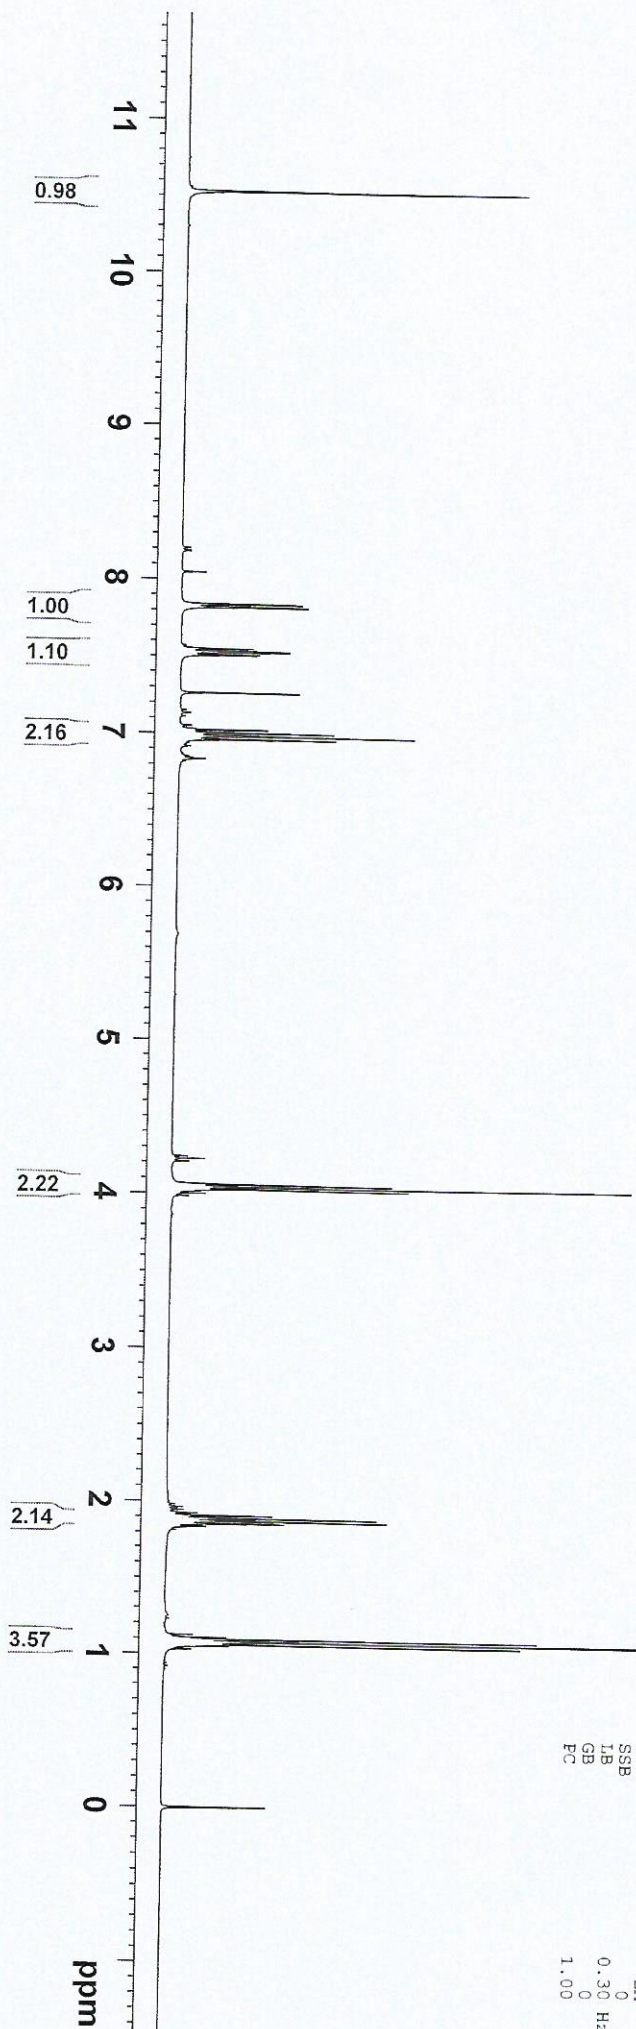

CHANNEL F1

NUC1	¹ H
P1	12.58 usec
PL1	0.00 dB
PL1W	10.87646866 W
SFO1	400.1324710 MHz
SI	32768
SF	400.1300091 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	1.00

NAME	Sep06-2015
EXPNO	14
PROCNO	1
Date_	20150906
Time	12.23
INSTRUM	spect
PROBHD	5 mm PABBO BB-
PULPROG	zgpg30
TD	65536
SOLVENT	CDCl3
NS	8
DS	2
SWH	8278.146 Hz
FIDRES	0.126314 Hz
AQ	3.9584243 sec
RG	181
DW	60.400 usec
DE	6.50 usec
TE	297.9 K
P1	1.00000000 sec
TD0	1