


501 616-45-5,85%,base,1.0,peak

Sample Name:	616-45-5,85%,base,1.0,peak	Injection Volume:	10.0
Vial Number:	321	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	215
Control Program:	0928-1	Bandwidth:	1
Quantif. Method:	DL	Dilution Factor:	1.0000
Recording Time:	2015-8-5 13:46	Sample Weight:	1.0000
Run Time (min):	16.34	Sample Amount:	1.0000

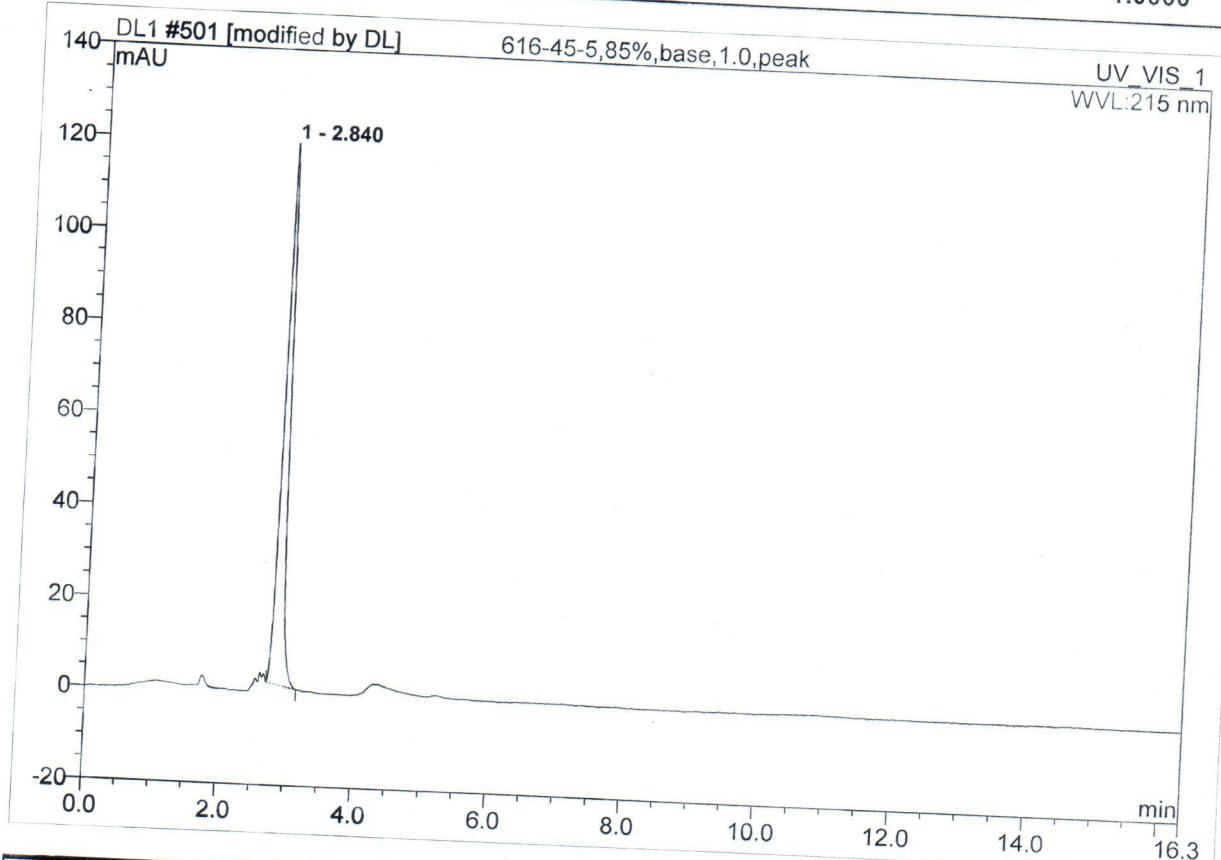

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	2.84	n.a.	117.776	12.197	100.00	n.a.	BMB
Total:			117.776	12.197	100.00	0.000	