

Display Report

Analysis Info


Analysis Name D:\Data\test\0318\lilaliting-Z_3_01_882.d
Method 882.m
Sample Name lilaliting-Z
Comment

Acquisition Date 3/18/2014 3:00:42 PM

Operator bruker
Instrument amaZon SL

Acquisition Parameter

Ion Source Type	ESI	Ion Polarity	Positive	Alternating Ion Polarity	off
Mass Range Mode	UltraScan	Scan Begin	70 m/z	Scan End	1000 m/z
Capillary Exit	140.0 V	n/a	n/a	Trap Drive	50.6
Accumulation Time	3530 μ s	Averages	5 Spectra	Auto MS/MS	off

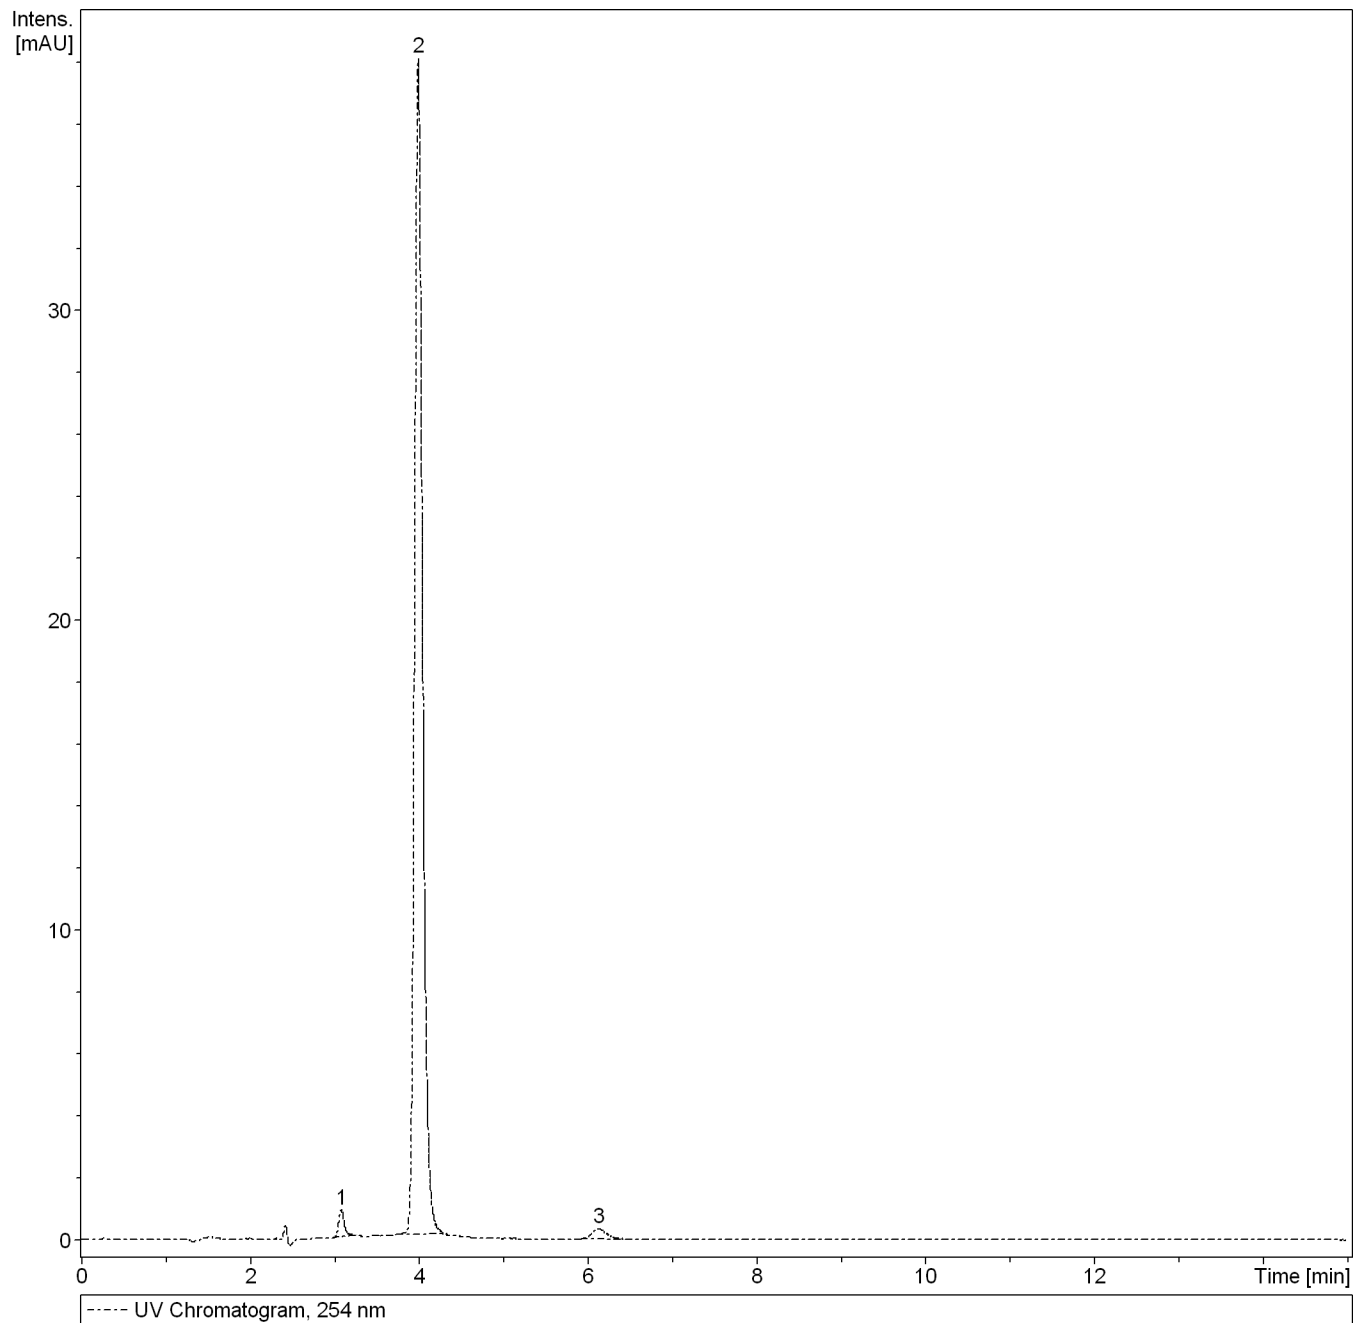

Display Report

#	RT [min]	Area	Area Frac. %
1	3.1	4.0590	1.6
2	4.0	250.4738	96.8
3	6.1	4.1611	1.6

Display Report

Analysis Info

Analysis Name D:\Data\test\0318\lilaliting-Z_3_01_882.d
Method 882.m
Sample Name lilaliting-Z
Comment

Acquisition Date 3/18/2014 3:00:42 PM

Operator bruker
Instrument amaZon SL

Acquisition Parameter

Ion Source Type	ESI	Ion Polarity	Positive	Alternating Ion Polarity	off
Mass Range Mode	UltraScan	Scan Begin	70 m/z	Scan End	1000 m/z
Capillary Exit	140.0 V	n/a	n/a	Trap Drive	50.6
Accumulation Time	3530 μ s	Averages	5 Spectra	Auto MS/MS	off

